FUJIFILM

Transrectal Probe

EUP-U533

INSTRUCTION MANUAL

Notes for operators and responsible maintenance personnel
★ Please read through this Instruction Manual carefully prior to use.
★ Keep this Instruction Manual together with the system with care to make it available anytime.

FUJIFILM Healthcare Corporation

Q1E-EP0397-15


© FUJIFILM Healthcare Corporation 2021. All rights reserved.

CE 0197

Manufacturer:



FUJIFILM Healthcare Corporation
2-1, Shintoyofuta, Kashiwa-shi, Chiba, 277-0804
Japan
+81-4-7131-4151
https://www.fujifilm.com/fhc/en



FUJIFILM Healthcare Deutschland GmbH
Otto-von-Guericke-Ring 3
D-65205 Wiesbaden, Germany



FUJIFILM Healthcare Logistics and Services
Zweigniederlassung der FUJIFILM Healthcare
Europe Holding AG
Otto-von-Guericke-Ring 3
D-65205 Wiesbaden, Germany



FUJIFILM Healthcare UK Ltd.
1 Davy Close, Park Farm Industrial Estate
Wellingborough, Northamptonshire, NN8 6XX,
United Kingdom

Local Distributor:

About this manual

This instruction manual contains safety precautions, the inspection, the operation procedure and the reprocessing procedure of the EUP-U533. Please read this manual thoroughly to ensure the safety operation. If you have any questions concerning the operation of the probe, please contact a service support.

The Symbols
The following conventions are used throughout the manual to denote special emphasis.

WARNING: "Warning" indicates the presence of a hazard which may result in severe personal injury, substantial property damage, or death if the warning is ignored.

CAUTION: "Caution" indicates the presence of a hazard which will or can cause minor personal injury or property damage if the caution is ignored.

NOTICE: "Notice" indicates information of installation, operation, or maintenance, which is important, but not hazard related.


Graphical Symbols for Use in Labeling of our company's Ultrasound Probes

Refer to the following table about the meanings of them.

Explanation of Symbol	Symbol	Descriptive Content
Manufacturer Company Name and Address		FUJIFILM Healthcare Corporation 2-1, Shintoyofuta, Kashiwa-shi, Chiba 277-0804 Japan +81-4-7131-4151 https://www.fujifilm.com/fhc/en
Authorized Representative in The European Community		FUJIFILM Healthcare Deutschland GmbH Otto-von-Guericke-Ring 3 D-65205 Wiesbaden, Germany
Keep away from Sunlight		Store the probe in a cool place and keep away from high temperature, high humidity, or direct sunlight.

Definition of symbol

The following symbol is also used for our company's Ultrasound Probes.

Location	Symbol	Definition
Probe connector Storage case	CE 0197	This instrument complies with Directive 93/42/EEC relating to Medical Device and Directive 2011/65/EU relating to RoHS
Probe connector	IPX7	IPX7 mark See section 1.5.
Probe connector		Type BF APPLIED PART
Probe connector		General warning sign
Probe connector		Warning; dangerous voltage
Contains or presence of natural rubber latex		Contains or presence of natural rubber latex
Do not reuse		Do not reuse
Probe connector		Caution; Biohazard
Probe connector		Follow the instruction manual to operate this instrument. If not avoided, may result in injury, property damage, or the equipment trouble.
Probe connector		Upper Limit of Temperature; The probes that are applicable to Ethylene Oxide Gas Sterilization use symbol of "Upper Limit of Temperature: 55 degrees".
Probe connector		Do not waste the instrument as general waste. Comply with a local regulation.
Probe connector	MD	Medical device
Probe connector	Rx Only	By prescription only. U.S. Federal Law restricts this device to sale on order of a physician only.
Probe connector Storage case	#	MODEL NUMBER
Probe connector Storage case	SN	SERIAL NUMBER

Probe connector Storage case		UNIQUE DEVICE IDENTIFIER
Probe connector Storage case		MANUFACTURER
Storage case		The importer for EEA: European Economic Area region is represented according to European Union Directives 93/42/EEC and 2011/65/EU.
Storage case		DATE OF MANUFACTURE The number under the mark indicates the year and month of manufacture. (in case of 2021-04) COUNTRY OF MANUFACTURE The character in the mark is the country of manufacture code defined by the International Organization for Standardization. (in case of JAPAN)
Storage case		AUTHORISED REPRESENTATIVE IN THE EUROPEAN COMMUNITY

CONTENTS

Page

1 Introduction ····· 1
1.1 Features ····· 1
1.2 Intended Use ····· 1
1.3 Components ····· 2
1.4 Accessories (Option) ····· 3
1.5 Construction ····· 4
2 Inspection before Use ····· 5
2.1 Inspection for Appropriate Connection ····· 5
2.2 Inspection for Material Surface ····· 5
3 Operation Procedure ····· 6
4 Option of EUP-U533 ····· 11
4.1 Magnetic sensor (EZU-RV2S) ····· 11
4.2 Magnetic sensor (EZU-RV3S) ····· 15
5 Cleaning, Disinfection and Sterilization ····· 18
5.1 Point of use (Pre-cleaning) ····· 21
5.2 Containment and transportation ····· 22
5.3 Manual Cleaning and disinfection ····· 22
5.4 Drying ····· 26
5.5 Inspection ····· 27
5.6 Packaging ····· 27
5.7 Sterilization ····· 28
5.8 Storage ····· 30
6 Cleaning, Disinfection and Sterilization of EZU-PA3U ····· 31
6.1 Point of use (Pre-cleaning) ····· 32
6.2 Containment and transportation ····· 32
6.3 Manual Cleaning and disinfection ····· 32
6.4 Automated cleaning and disinfection ····· 34
6.5 Drying ····· 35
6.6 Inspection ····· 35
6.7 Packaging ····· 35
6.8 Sterilization ····· 36
6.9 Storage ····· 36
7 Maintenance and Safety Inspection ····· 37
7.1 Daily Inspection ····· 37
7.2 Storage ····· 37
8 Safety Precautions ····· 38
9 Specifications ····· 40
9.1 Probe ····· 40
9.2 Puncture Guide Fixture ····· 41
9.3 Suppliers List ····· 42
10 Disposal of the probe ····· 42

1 Introduction

1.1 Features

The Transrectal probe of Model EUP-U533 has convex array electronic scanning type and linear array electronic scanning. The acoustic output of this probe when connected to ultrasound scanner was measured according to the IEC60601-2-37 standard. The table of measured acoustic output data is contained in the operational manual of each ultrasound scanner. This probe is categorized in class IIa according to Directive 93/42/EEC. According to IEC60601-1 the probe is classified as type BF.

⚠ WARNING

When using the needle cannula of the electrosurgical unit while using the Puncture Guide Fixture as a guide, be careful not to damage the insulation coating of the needle cannula.
[When inserting or removing the needle cannula into or from the Puncture Guide Fixture, you may damage the insulation coating of the needle cannula, which may cause a burn to tissue contacting the exposed section of the insulation coating.]

1.2 Intended Use

The Transrectal Probe EUP-U533 is designed for observation and diagnosis of the following regions mainly by connecting with our company's ultrasound diagnostic scanner.

- Transrectal
- Biopsy (with a Puncture Guide Fixture)

⚠ WARNING

Never use the probe for following regions.
1) The heart (Do not contact directly.)
2) The eyeball

1.3 Components

Components of the EUP-U533 are as follows:

1) Transrectal Probe EUP-U533 ····· 1 piece
2) Puncture Guide Fixture EZU-PA3U ····· 1 piece
3) Syringe kit ····· 1 set
   a) Extension Tube ····· 1 piece
   b) Three-way cock ····· 1 piece
   c) Syringe ····· 1 piece
4) Balloon Kit part number: 1450303A ····· 1 set
   a) Balloon ····· 12 pieces
   b) Rubber Band ····· 24 pieces
5) Instruction Manual ····· 1 copy

⚠ CAUTION

Sterilization has not been made to the probe, Puncture Guide Fixture EZU-PA3U and balloon kit shipped from the factory. Prior to use of the probe, be sure to clean, disinfect and sterilize it.

⚠ WARNING



The balloon kit is made by latex. The latex may cause such allergic reactions as itching, rubor, urticaria, swelling, fever, anhelation, wheezing, depression of blood pressure, shock and so on. For the patients suspected of latex allergy, do not use the latex-containing medical devices. If you observe any of above-mentioned symptoms in your patient during the operation, stop the use of the latex-containing medical devices immediately and take an appropriate treatment to the patient.

⚠ CAUTION

Do not hold the needle cannula of the electrosurgical unit with metal tweezers, forceps, and the like.
[Doing so may damage the insulation section of the needle cannula, and may cause a burn to a non-treated area.]

1.4 Accessories (Option)

1.4.1 Probe cover (Disposable)



To protect the probe against contamination, use only lubrication free probe cover, which is dry type. Lubrication may cause a deterioration of the probe surface. And latex rubber may create allergic reactions, use of non-allergic probe cover is strongly recommended.
Take care for the handling of used probe cover.

1.4.2 Magnetic Sensor Attachment

Magnetic sensor attachment is used for Real-time Virtual Sonography (RVS). By using the attachment, the magnetic sensor is attached to the probe that is connected to our company's ultrasound scanner.


1.4.3 Spacer for EZU-RV2S

Spacer for EZU-RV2S is used for Real-time Virtual Sonography (RVS) with an EZU-RV2S. By using the Spacer, the magnetic sensor for EZU-RV2S is attached to the Magnetic sensor attachment.

⚠ CAUTION

Sterilization has not been made to the Magnetic sensor attachment and the Spacer for EZU-RV2S shipped from the factory. Prior to use of the probe, be sure to clean, disinfect, and sterilize it.

1.5 Construction

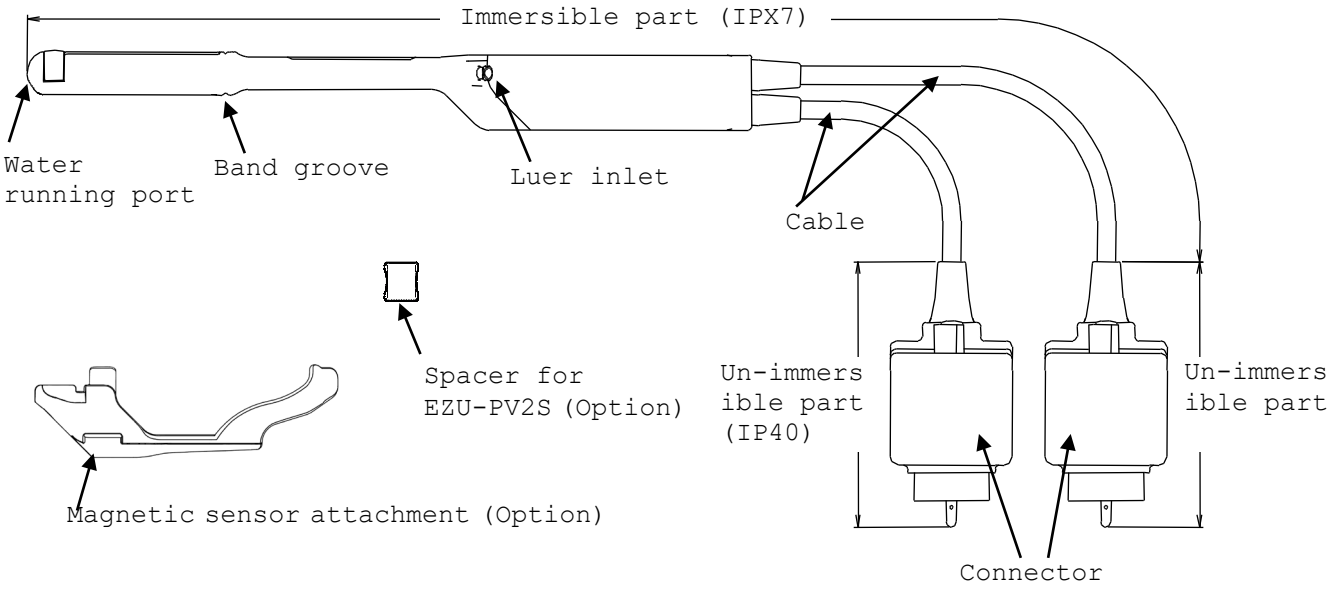

Immersible part: This part can be immersed in disinfectant solution and also can be cleaned by water.

Un-immersible part: This part should not be immersed in disinfectant solution and also can not be cleaned by water.

Fig.1 External view

2 Inspection before Use

Prior to use, the probe, the Puncture Guide Fixture and accessories must be carefully inspected that they are appropriate for use. If you find any damage, do not use them and contact one of our company and/or distributor's offices immediately.

2.1 Inspection for Appropriate Connection

2.1.1 Confirm that the system is correctly operating. Refer to the instruction manual for the Main unit.

2.1.2 Do not attach or connect unauthorized devices or instruments on the probe, such as unauthorized biopsy attachments.

2.1.3 Confirm that the Puncture Guide Fixture and software version and then settings of the scanner are appropriate for the probe. Attach the Puncture Guide Fixture on the probe. Set the main unit to display “Needle guide line”. (Refer to the operation manual for the main unit.) Keep the probe head in the water and insert a puncture needle in the Puncture Guide Fixture. Then, confirm that the needle is inserted smoothly and the echo of the needle is displayed on the dot line “Needle guide line” on the monitor.

2.2 Inspection for Material Surface

2.2.1 Visually inspect the surface of the probe head, housing and cable for any crack, scratch or denaturalization.

2.2.2 Visually inspect the envelope of the Puncture Guide Fixture for any break, deformation or denaturalization. If you find any damage, do not use the Puncture Guide Fixture.

2.2.3 Visually inspect the Magnetic sensor attachment and the Spacer for EZU-RV2S for any crack, deformation or denaturalization. If you find any damage, do not use the Spacer for EZU-RV2S.

2.2.4 Check whether there is the Spacer for EZU-RV2S nearby when use RVS.

⚠ CAUTION

The Spacer for EZU-RV2S is small, please do not lose the Spacer.

3 Operation Procedure

1) Confirm that the probe is disinfected. In case of using Real-time Virtual Sonography (RVS), confirm that the Magnetic sensor attachment and the spacer are disinfected and if necessary sterilized. In case of using RVS with EZU-RV2S, confirm that the Spacer for EZU-RV2S is also disinfected and if necessary sterilized.
2) It is recommended to use a disposable probe cover for preventing a patient from infection and the probe cover should be allergy free material to avoid allergic reaction.
3) Connect the probe to the Ultrasound diagnostic scanner and operate the scanner and adjust the image according to the instruction given in the operation manual for Ultrasound diagnostic scanner.
4) The relationship between the direction of the probe and the right-left orientation mark on the image is shown in Fig.2-1 and Fig.2-2.

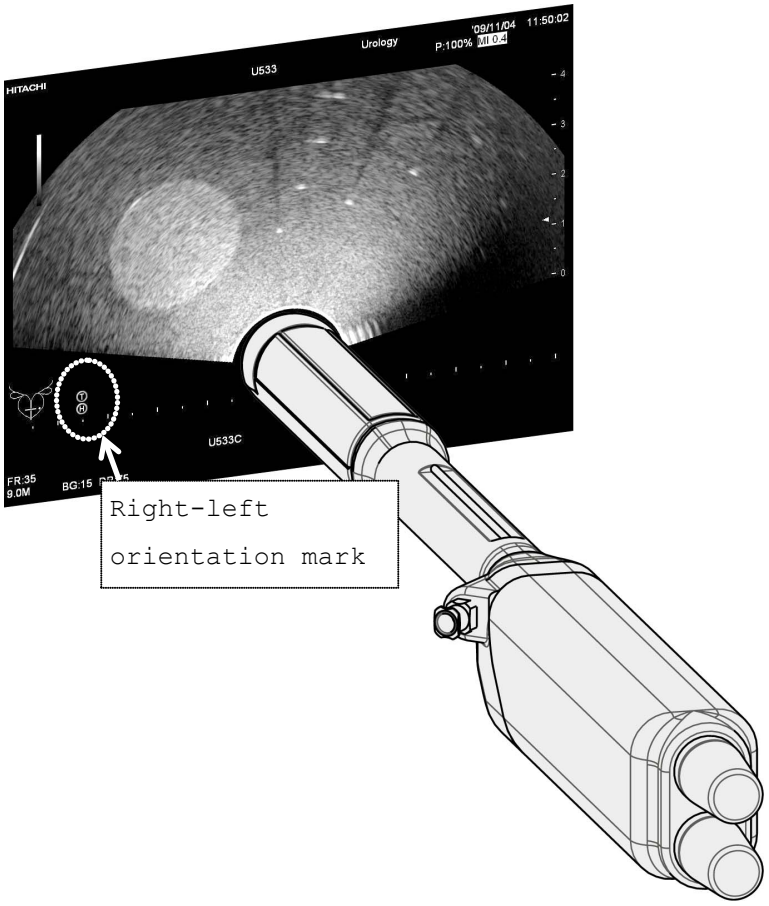


Fig.2-1 The relationship between the direction of the probe and the Right-left Orientation Mark in Convex US image

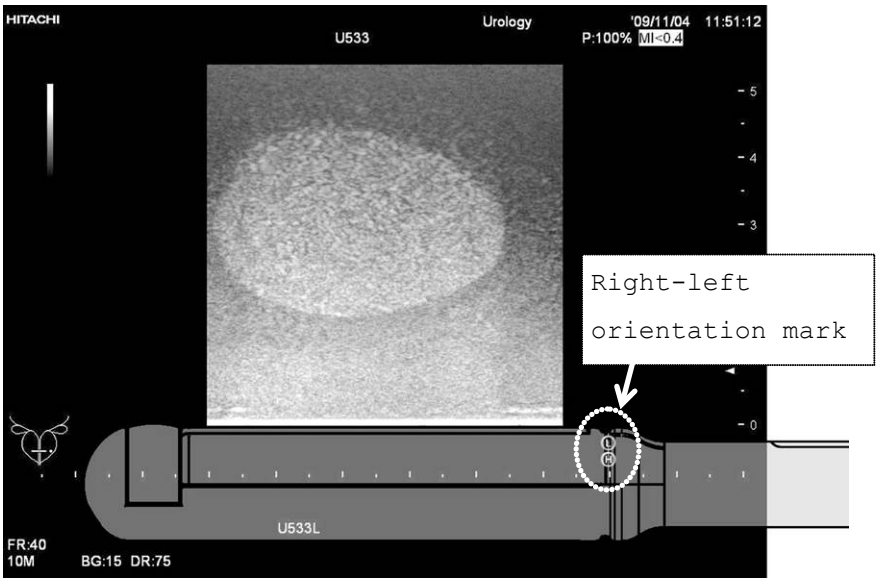


Fig.2-2 The relationship between the direction of the probe and the Right-left Orientation Mark in Linear US image

5) In prior to starting the examination, prepare below mentioned materials.
   - Balloon
   - Rubber band
   - Extension tube
   - Three-way cock
   - Syringe
   - Physiological saline
6) In prior to starting the examination, finish below mentioned preparations.
   (1) Cover the probe with the balloon from the top of probe.
   (2) Tighten the balloon by the rubber band.
   (3) Connect the extension tube, three-way cock, syringe filled with physiological saline to the Luer inlet of probe and fill the balloon with physiological saline. In case of remaining the air in the balloon, deflate the air bubble with the syringe.
   (4) Return physiological saline to the syringe.

7) Perform the examination under following procedures.
   (1) Insert the probe into patient's body.
   (2) Pour an adequate volume of physiological saline into the balloon.
   (3) Perform the examination. Regarding adjustments of image and so on, refer to the operating manual of the scanner to which the probe is connected.
   (4) When the examination is finished, return physiological saline in the balloon to the syringe before removing the probe from the body.
   (5) Remove the probe from the body.
8) After using the probe, clean and disinfect or sterilize the probe immediately and using RVS, also clean and disinfect or sterilize the Magnetic sensor attachment.
   In case of using RVS with an EZU-RV2S, also clean and disinfect or sterilize the Spacer for EZU-RV2S.
9) Store the probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S in the environment indicated in "7. Maintenance and Safety Inspection".

⚠ CAUTION

The needle guideline can be displayed on US image when the perineal prostate paracentesis would be operated by this probe with the Puncture Guide Fixture EZU-PA3U.

When the needle guideline is displayed, numeric value in the upper right is displayed on US image. This numeric value means the distance between the surface of acoustic lens and the needle guideline. Refer to the following image. About how to display the needle guideline, refer to the instruction manual of the ultrasound scanner that the ultrasound probe is connected to.


The numeric value on the image corresponds to the numeric value that is engraved to Puncture Guide Fixture EZU-PA3U. For example, when the movable part for guiding the needle is fixed to 10mm position, adjust the numeric value in the upper right on US image to 10mm. The movable part for guiding the needle and the needle guideline can move from 10mm to 50mm per 5mm. additionally, note that display position of the numeric value is different by ultrasound scanner.

About how to adjust the needle guideline, refer to the instruction manual of the ultrasound scanner that the ultrasound probe is connected to.

Before use, make sure there is no damage to the surface to which the needle cannula is attached, and the Puncture Guide Fixture works properly.

⚠ CAUTION

The actual distance from the surface of acoustic lens to the needle guideline is approximate 3mm shorter than the numeric value in the upper right on US image. However, the needle echo image corresponds with the needle guideline. So perform the paracentesis by using the needle guideline as rough indication.

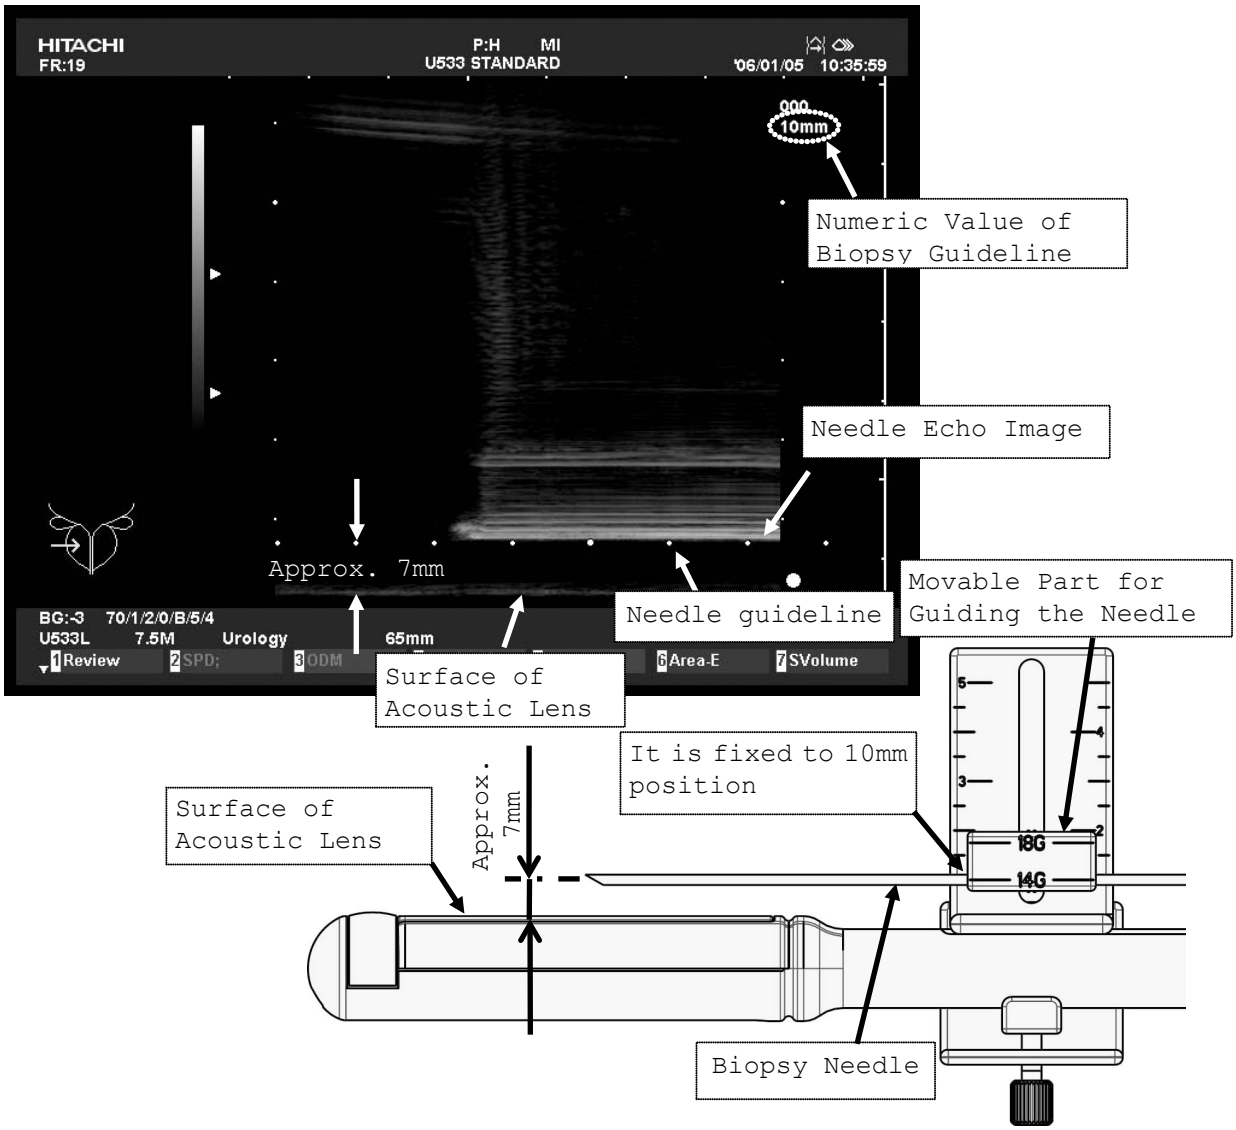

4 Option of EUP-U533

In case of using RVS (Real-time Virtual Sonography), confirm that type of the magnetic sensor. There are two types of the magnetic sensors for EUP-U533, EZU-RV2S and EZU-RV3S.
EZU-RV2S and EZU-RV3S are shown in Fig.3 and Fig.8.
The use of the EUP-U533 with the magnetic sensor enables the user to perform RVS (Real-time Virtual Sonography).

4.1 Magnetic sensor (EZU-RV2S)

Magnetic sensor as shown in Fig.4 is for the EUP-U533.

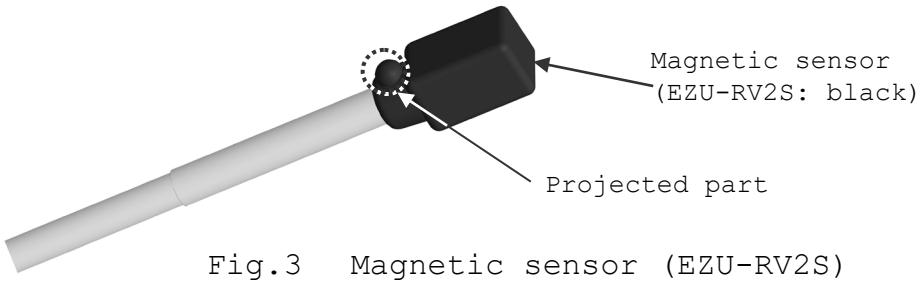


Fig.3 Magnetic sensor (EZU-RV2S)

4.1.1 How to attach the Magnetic sensor

The procedure of attaching the Magnetic sensor is as follow.

1) Confirm that the Magnetic sensor attachment and the Spacer for EZU-RV2S are disinfected and if necessary sterilized.
2) Connect the probe, operate the ultrasound diagnostic scanner, and adjust the image according to the instructions given in the operation manual for the ultrasound diagnostic scanner.
3) To use RVS (Real-time Virtual Sonography), attach the magnetic sensor as shown below.

a) Attach the Spacer for EZU-RV2S to the Magnetic sensor.
b) Insert the Magnetic sensor into the Magnetic sensor attachment at the correct direction as shown in Fig.4.

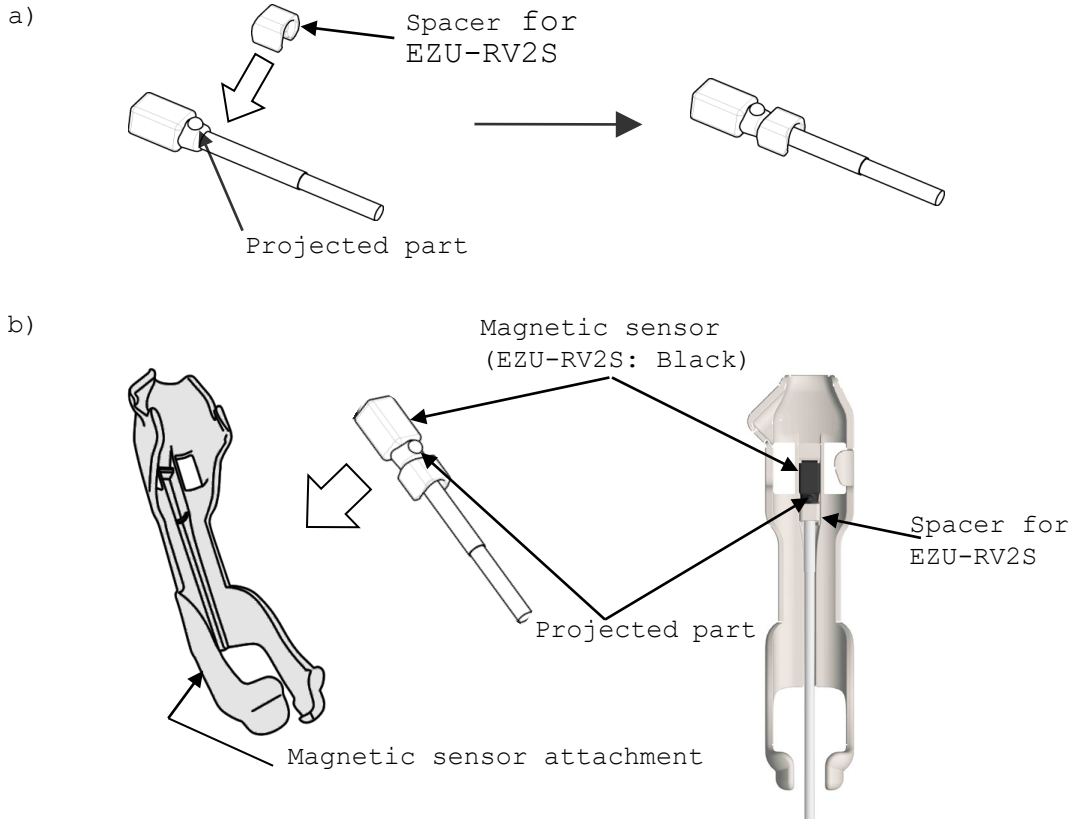


Fig.4 How to attach the Magnetic sensor

⚠ CAUTION

1) Never attach the Magnetic sensor attachment to the probe in the incorrect direction, otherwise it may result in false diagnosis.
2) Never forget to attach the Spacer for EZU-RV2S when using RVS with Magnetic sensor EZU-RV2S, otherwise it may result in false diagnosis.

c) Attach the Magnetic sensor attachment to the probe as shown in Fig.5.

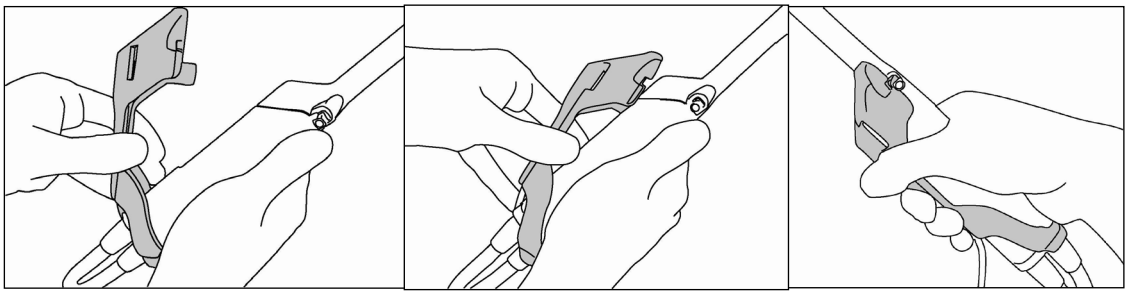


Fig.5 How to attach the Magnetic sensor attachment

⚠ CAUTION

Do not put your fingers between the Magnetic sensor attachment and the probe when attaching the Magnetic sensor attachment to the probe.

4.1.2 How to release the Magnetic sensor

The procedure of releasing the Magnetic sensor is as follow.

1) Detach the Magnetic sensor attachment from the probe as shown Fig.6.

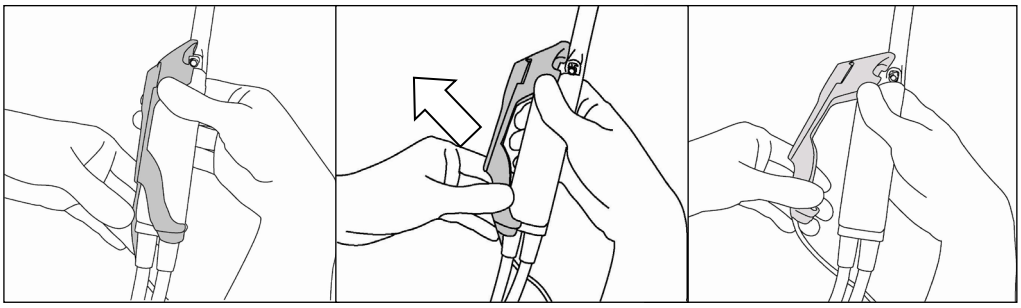


Fig.6 How to release the Magnetic sensor attachment from the probe

2) Detach the magnetic sensor and the Spacer for EZU-RV2S from the Magnetic sensor attachment as shown Fig.7.

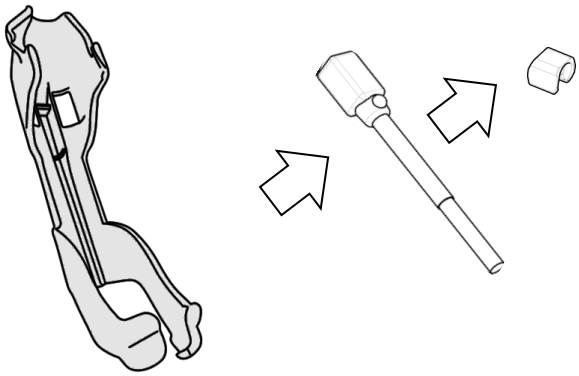


Fig.7 How to release the Magnetic sensor from the Magnetic sensor attachment

⚠ CAUTION

Clean , disinfect and sterilize the Magnetic sensor attachment and the Spacer for EZU-RV2S before the first use as there are not sterilized in the factory.

4.2 Magnetic sensor (EZU-RV3S)

Magnetic sensor (EZU-RV3S) as shown in Fig.8 is the magnetic sensor for EUP-U533.

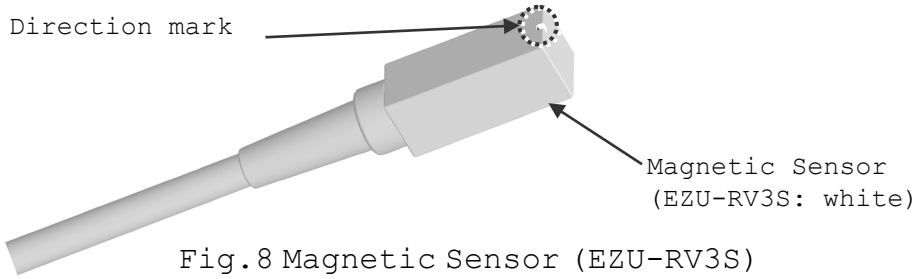


Fig.8 Magnetic Sensor (EZU-RV3S)

4.2.1 How to attach the Magnetic sensor

The procedure of attaching Magnetic sensor is as follow.

1) Confirm that the Magnetic sensor attachment and the Spacer for EZU-RV3S are disinfected and if necessary sterilized.
2) Connect the probe, operate the ultrasound diagnostic scanner, and adjust the image according to the instructions given in the operation manual for the ultrasound diagnostic scanner.
3) To use RVS (Real-time Virtual Sonography), attach the magnetic sensor as shown below.

a) Insert Magnetic sensor into the Magnetic sensor attachment at the correct direction as shown in Fig.9.

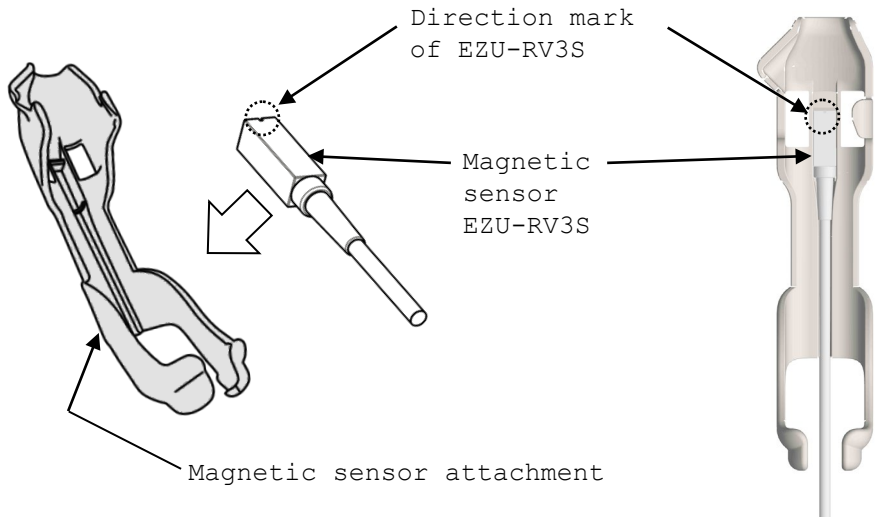


Fig.9 How to attach the Magnetic sensor

⚠ CAUTION

Never attach the Magnetic sensor attachment to the probe at the incorrect direction, otherwise it may result in false diagnosis.

b) Attach the Magnetic sensor attachment to the probe as shown in Fig.10.

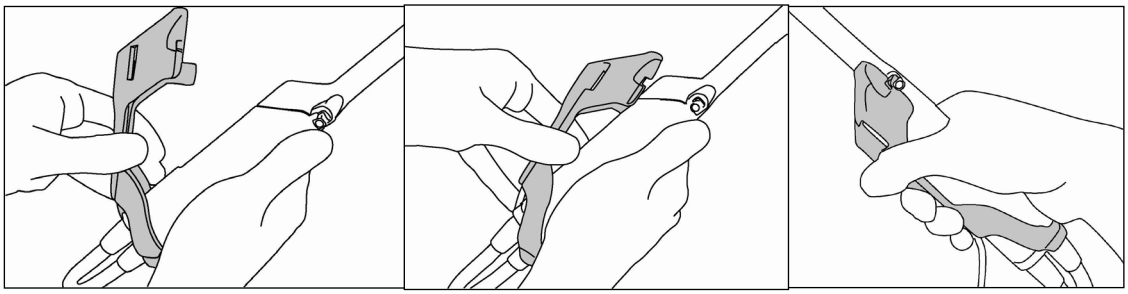


Fig.10 How to attach the Magnetic sensor attachment

⚠ CAUTION

Do not put your fingers between the Magnetic sensor attachment and the probe when attaching the Magnetic sensor attachment to the probe.

4.2.2 How to release the Magnetic sensor

The procedure of releasing the Magnetic sensor is as follow.

1) Detach the Magnetic sensor attachment from the probe as shown Fig.11.

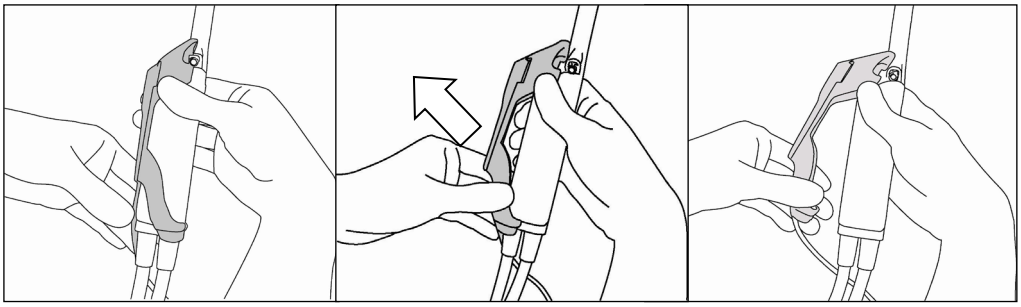


Fig.11 How to release the Magnetic sensor attachment from the probe

2) Detach the magnetic sensor from the Magnetic sensor attachment as shown Fig.12.

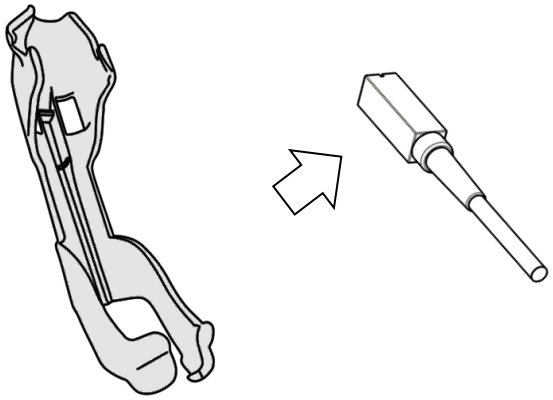


Fig.12 How to release the EZU-RV3S from the Magnetic sensor attachment

⚠ CAUTION

Clean , disinfect and sterilize the Magnetic sensor attachment before the first use as there are not sterilize in the factory.

5 Cleaning, Disinfection and Sterilization



The probe and accessory must be reprocessed after each use. Refer to the reprocessing instruction in this chapter.

WARNINGS	- Particular attention is required when reprocessing probes with lumen. - The probe is delivered unsterile. Prior to the first use, reprocess the probe. - Temperature should not exceed 60°C (140°F) during reprocessing. - Probe connector is not water resistant.
Limitations on reprocessing	The probe is not completely submersible. The immersible part is shown in Fig.1. The un-immersible part should be disinfected by wipe disinfection.
Transportation before using	The probe should be packed in a sterile pouch or container to transport from Central Sterile Supply Department (CSSD) to an operating room. Be careful not to damage the sterile pouch or container during transportation.


Levels of reprocessing requirements:

Depending on the application of the product and with regard to risk evaluation, the user has to classify the medical device according to the current Medical Device Directive for processing of medical devices as uncritical, semi-critical or critical. Supporting information concerning this topic is listed in the table below. The user is responsible for correct classification of the medical device.

Classification	Definition	Processing
uncritical	Application part only contacts intact and uninjured skin	Cleaning Disinfection
semicritical	Application part contacts mucosa (intracavitary application)	Cleaning Disinfection (Disinfectant with virucidal effect)
critical	Application part contacts intracorporeal tissue directly (operative application)	Cleaning Disinfection (Disinfectant with virucidal effect - minimum) Sterilization

According to the intended use, EUP-U533 is classified as semicritical.

The flowchart of the reprocessing process of this probe is as follows.

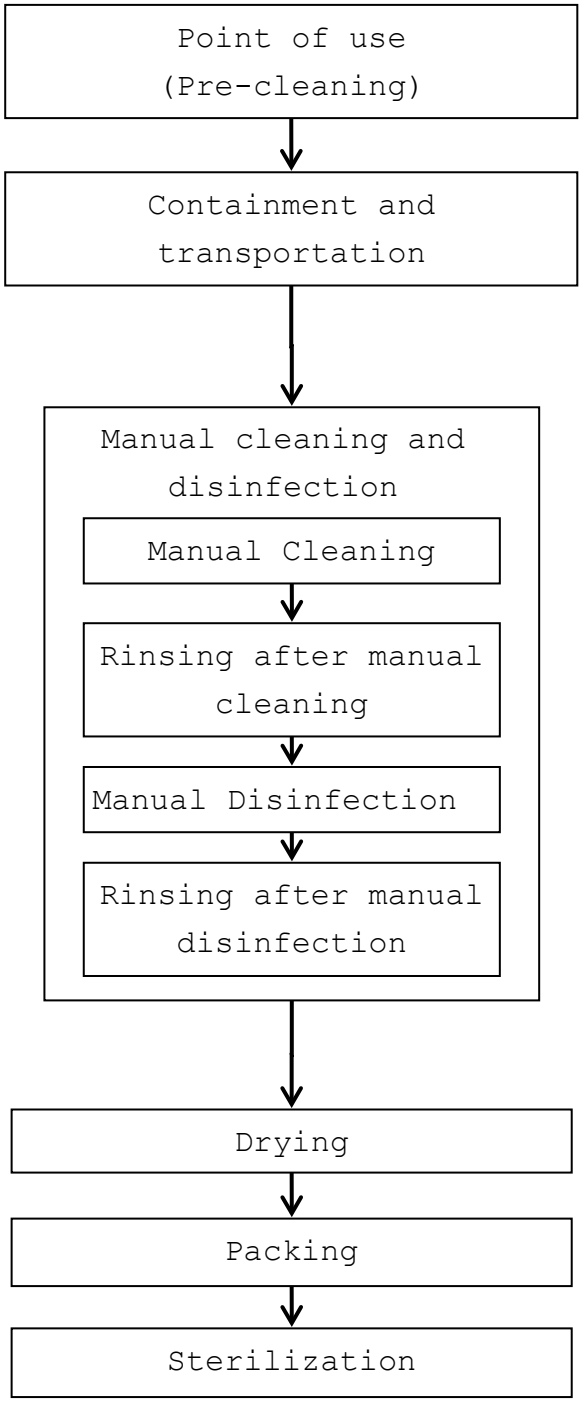

5.1 Point of use (Pre-cleaning)

Point of use (Pre-cleaning)

Pre-cleaning should be done immediately after each use. The procedure is as follows:

A) EUP-U533


1) Remove the protective cover.
2) Flush the lumen of the probe directly after use with 50 ml deionized water/tap water using a 50 ml syringe (adaptation of the syringe to the Luer inlet of the probe).
3) Clean the probe of all patient's blood or fluid with running tap water until the surface of the probe looks visually clean.
4) Wipe the whole surface of the probe with gauze pad and remove superficial visible impurities.

B) Magnetic sensor attachment and Spacer for EZU-RV2S

1) Remove the Magnetic sensor attachment and the magnetic sensor from the probe. Remove the Spacer for EZU-RV2S from the magnetic sensor if the sensor is EZU-RV2S.
2) Immerse the Magnetic sensor attachment and the Spacer for EZU-RV2S in sufficient amount of high quality tap water. Scrub them using soft cloth to remove all visible soil from their surface.


5.2 Containment and transportation

Putting the contaminated equipment into exclusive shock and damage proof container for transportation is recommended. It is recommended that instruments are reprocessed as soon as possible and not later than 4 hours after usage.

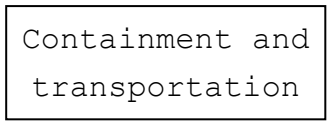

5.3 Manual Cleaning and disinfection

<u>Prepare following items before manual cleaning and disinfection:</u>

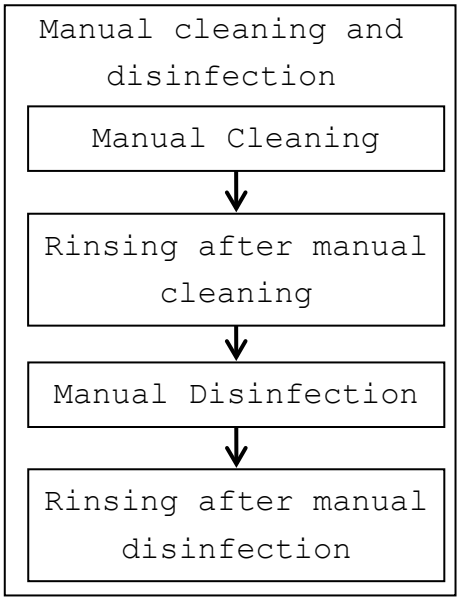

a) Detergent: Cidezyme

   (Johnson & Johnson, #2258) or another cleaning agent with approved material compatibility for this medical device.

b) Disinfectant: Cidex OPA

   (Johnson & Johnson, # 20391) or another disinfectant with approved material compatibility for this medical device.

c) Cleaning brushes if applicable, i.e. Olympus Model Nr. BW-400L or Interlock model REF 09099 (cleaning the lumen of the water channel)

d) Two tanks, one for cleaning and one for disinfection - optional:

   - 1 additional tank for rinsing with deionized/tap water (sufficient size for immersion of the immersible part of the probe at full length)

e) Syringe 50 ml with Luer-lock

f) Soft, fluff free cloth or single use towel

g) Personal protective equipment (gloves, water repellent protective skirt, face protection mask or protective glasses, see also instructions of the manufacturer for the detergent and the disinfectant)

Manual Cleaning:

Prepare the detergent solution in a tank with cold water (please follow the instructions of the detergent manufacturer regarding application, dilution and contact time).

A) EUP-U533

1) The temperature of the detergent solution should be between 15-30°C (59-86°F), concentration is 1.6%. Please note the minimum contact time of the detergent in the manufacturer's instruction. If a differing detergent is used, please also note the approved material compatibility for the medical device.

2) Immerse the immersible part of the probe without connector into the diluted detergent solution. Wipe the immersible part of the probe under the surface of the detergent solution with a soft cloth to remove all visible soil.

3) Use the syringe via the Luer inlet to fill and rinse the lumen with the detergent solution. The lumen of the probe is rinsed 5 times under the surface of the detergent solution with 50 ml diluted detergent. Drain the detergent out of the lumen by using the syringe. Afterwards, remove the syringe from the probe.

4) Insert the cleaning brush into the lumen via the Luer inlet until the end of the channel is reached. Brush the whole length of the lumen at least 5 times. In addition all immersible parts of the probe are wiped with a soft cloth until visually clean.

⚠ CAUTION

The inside of the water channel is very sensitive, so if the water channel is cleaned, cleaning brush should be operated carefully. If brushing is rough, water channel may suffer serious damage.

5) Rinse the lumen 5 times with the detergent solution by using the syringe.

6) The immersible part of the probe should be left in the detergent solution according to the specified contact time of the detergent manufacturer.

7) Wipe the un-immersible parts of the probe with a soft cloth dipped with the detergent solution.

8) Rinse the probe and the lumen with running tap water for 1 minute,

ensuring that the lumen is rinsed properly.
(alternatively: immerse the immersible part of the probe in a tray filled with tap water (see Fig.13) for 5 min. and rinse the lumen of the probe with 50 ml deionized water/tap water 5 times by using the syringe)

9) Visually check the outer surface of the probe for cleanness. If necessary, use magnifying glass for visually check. If there is still soil visible, repeat all above steps.

B) Magnetic sensor attachment and Spacer for EZU-RV2S

1) The temperature of the detergent solution should be between 15-30°C (59-86°F), concentration is 1.6%. Please note the minimum contact time of the detergent in the manufacturer's instruction. If a differing detergent is used, please also note the approved material compatibility for the medical device.

2) Immerse the magnetic sensor attachment and the Spacer for EZU-RV2S into the diluted detergent solution. Wipe them under the surface of the detergent solution with a soft cloth to remove all visible soil.

3) The Magnetic sensor attachment and the Spacer for EZU-RV2S should be left in the detergent solution according to the specified contact time of the detergent manufacturer.

4) Rinse the Magnetic sensor attachment and the Spacer for EZU-RV2S with running tap water for 1 minute. (alternatively: immerse them in a tray filled with deionized water/tap water (see Fig. 13) for 5 min.)

5) Visually check the outer surface of the Magnetic sensor attachment and the Spacer for EZU-RV2S for cleanness. If necessary, use magnifying glass for visually check. If there is still soil visible, repeat all above steps.

Manual disinfection:

A) EUP-U533

1) Prepare the disinfectant solution in a tank with cold water (please follow the instructions of the disinfectant manufacturer regarding application, concentration, microbiological efficiency, service life and contact time).

2) Confirm the concentration of the disinfectant before immersing the probe. Although Cidex® OPA does not need to be diluted, it is recommended to use test strips to verify the concentration. The test strips can indicate whether or not the concentration is above the Minimum Effective Concentration (MEC). Please also note the expiration date of the test stripes. Temperature of disinfectant solution should be minimum 20°C (68°F). The minimum contact time is 5 minutes. If a different disinfectant is used, follow the manufacturer's instructions. Please also consider the material compatibility for the medical device.

3) Immerse the immersible part of the probe into the disinfectant (see Fig. 13). Use the syringe via the Luer inlet to fill and rinse the lumen with the disinfectant solution. The lumen of the probe is rinsed 5 times under the surface of the disinfectant solution with 50 ml disinfectant. Set a clock to insure the recommended contact time which is 5 minutes. Note that air inside the lumen should be removed to disinfect properly.

4) Rinse the immersible part of the probe and the lumen of the probe with deionized water for 1 minute, ensuring that the lumen is rinsed properly.
(alternatively: immerse the immersible part of the probe in a tray filled with deionized water (see Fig. 13) for 5 min. and rinse the lumen of the probe with 50 ml deionized water 5 times by using the syringe)

5) Visually check the outer surface of the probe for leavings of the disinfectant. If necessary, repeat the rinsing.

B) Magnetic sensor attachment and Spacer for EZU-RV2S

1) Prepare the disinfectant solution as stated in the procedure for the probe.

2) Immerse the Magnetic sensor attachment and the Spacer for EZU-RV2S into the disinfectant (see Fig13). Set a clock to insure the recommended contact time which is 5 minutes.

3) Rinse the Magnetic sensor attachment and the Spacer for EZU-RV2S with deionized water for 1 minute. (alternatively: immerse them in a tray filled with deionized water (see Fig. 13) for 5 min.)

4) Visually check the outer surface of the Magnetic sensor attachment and the Spacer for EZU-RV2S for leavings of the disinfectant. If necessary, repeat the rinsing.

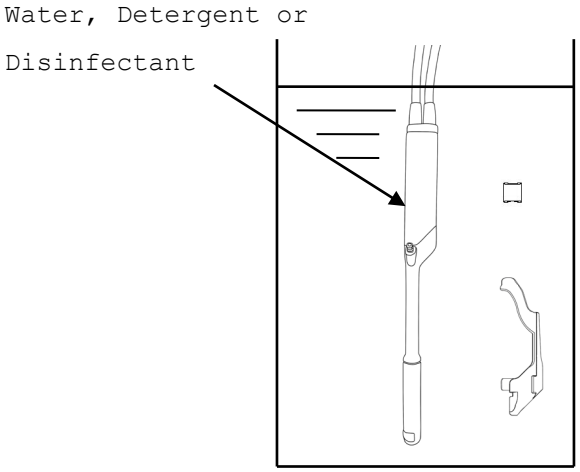


Fig.13 Immersion of the Probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S

5.4 Drying

Drying

1) Wipe the probe with a single-use, fluff-free wipe or towel to remove moisture from the surface of the probe.

2) Dry the lumen by applying compressed air. The compressed air should be filtered by a sterile filter that removes air particles of less than 0.2 µm. Dry until no visible moisture is left.

3) Dry the probe naturally in an ambient temperature between 15-30°C (59-86°F) for a minimum of 4 hours. Alternatively the probe can be dried using a drying heater at a temperature of less than 55°C (131°F).

5.5 Inspection

Inspect the equipment for any damage such as crack, scratch or deformation. Do not use it if any damage is found.

5.6 Packaging

Packaging

Pack the equipment in a sterile barrier such as Polypropylene fleece or transparent package made from Polyethylene film and Tyvek®, and then place it into a tray. The tray should be also covered with a sterile barrier.

Additionally the equipment can be placed on plastic mesh wires supplied for plasma sterilization and then packed as mentioned above.

The equipment can be packed in a simple or double packing.

Please note that the size of a sterile barrier should be large enough to be able to pack the equipment leaving sufficient space to seal it completely.

A sterile barrier should be sealed by an appropriate sealing machine and it is important to confirm that the package is sealed completely. If the sealing is not complete, pack and reseal again.

5.7 Sterilization

Sterilization

The probe and accessory can be sterilized using either ethylen oxide gas (EtO) sterilization or plasma sterilization (see table below).

Follow the manufacturer's instructions of the sterilizer regarding usage, temperature and sterilization-time.

The sterilization method and operating conditions are as follows.

Sterilization Method	Condition
Plasma Sterilization: STERRAD® 50, 100S or 200 (*)	Short Cycle
Plasma Sterilization: Sterrad® NX or 100NX (*)	Standard cycle
ETO Sterilization	➢ Gas Type: 10% EO/ 90% HCFC ➢ Temperature: 50-55°C 122-131°F ➢ Exposure Time: More than 120 minutes ➢ Pressurization: 162-200kPa Depressurization: 13-8kPa ➢ Relative humidity: 40-90% ➢ Aeration temperature: 53°C 127.4°F ➢ Aeration is minimum 12 hours

* STERRAD® systems are manufactured by "Johnson & Johnson"

⚠ CAUTION

1) Before performing sterilization, check that the operation data of sterilizer are in conjunction with min. and max. data applicable for the probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S.

2) Do not sterilize the probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S by Steam Autoclaving. If you autoclave them, they suffers serious damage and will be not functional.

The packaging procedure is as follows.

1) Put the probe into TYVEK pouch.

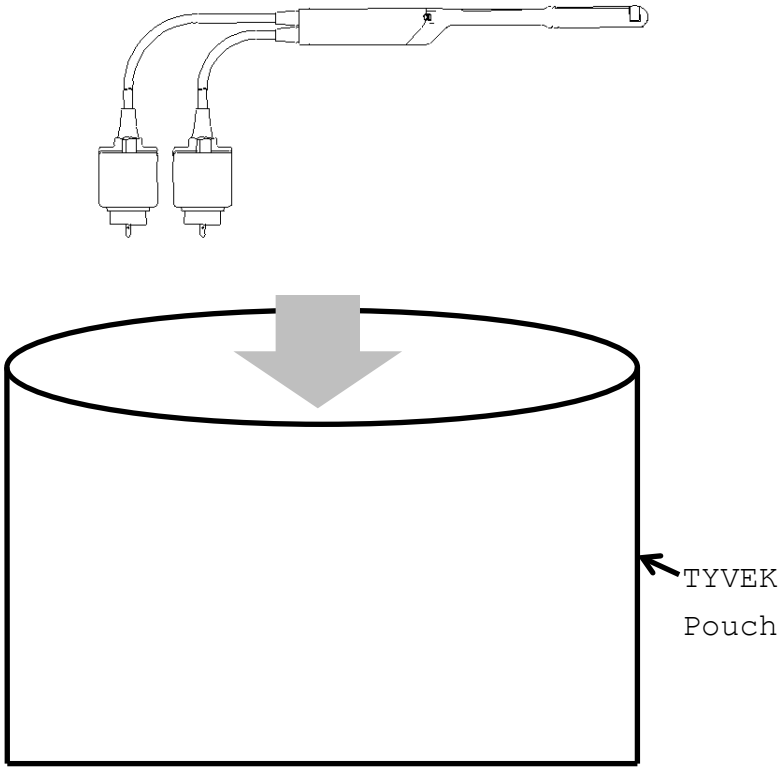


Fig.14 Packaging in the pouch

2) Seal the TYVEK Pouch using a heat sealer. Ensure that the seal is complete.

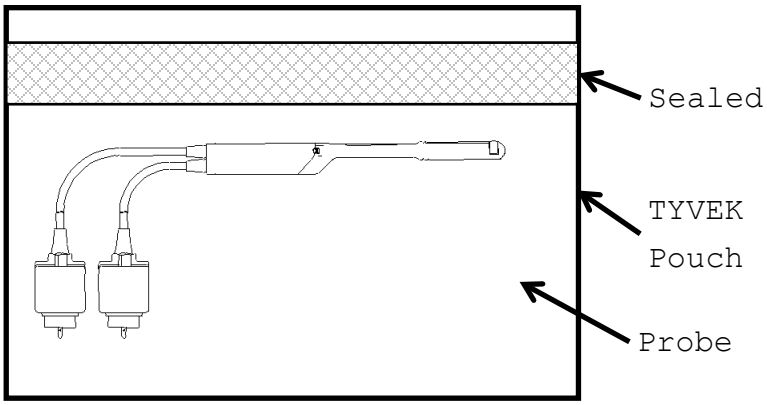


Fig.15 Sealing

3) Put the sealed pouch into a tray or plastic mesh wire for sterilization.

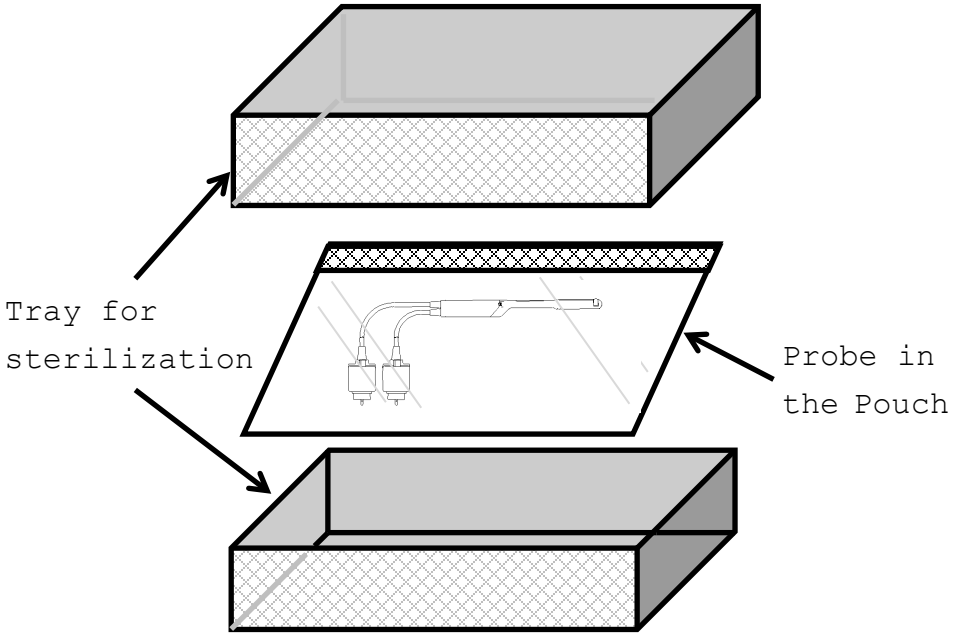


Fig.16 Packaging in a tray

5.8 Storage



Store the equipment in a cool, dustproof and dark, dry space to avoid high temperature, humidity and direct sunlight. Limitations for the time for sterilized equipment belong to package.


6 Cleaning, Disinfection and Sterilization of EZU-PA3U

EZU-PA3U must be reprocessed after each use. Refer to the reprocessing instruction in this chapter.

WARNINGS	EZU-PA3U is delivered unsterile. Prior to the first use, reprocess it.
Transportation before using	EZU-PA3U should be packed in a sterile pouch or container to transport from Central Sterile Supply Department (CSSD) to an operating room. Be careful not to damage the sterile pouch or container during transportation.

Levels of reprocessing requirements:
Refer to the chapter 5.

The flowchart of the reprocessing process of EZU-PA3U is as follows.

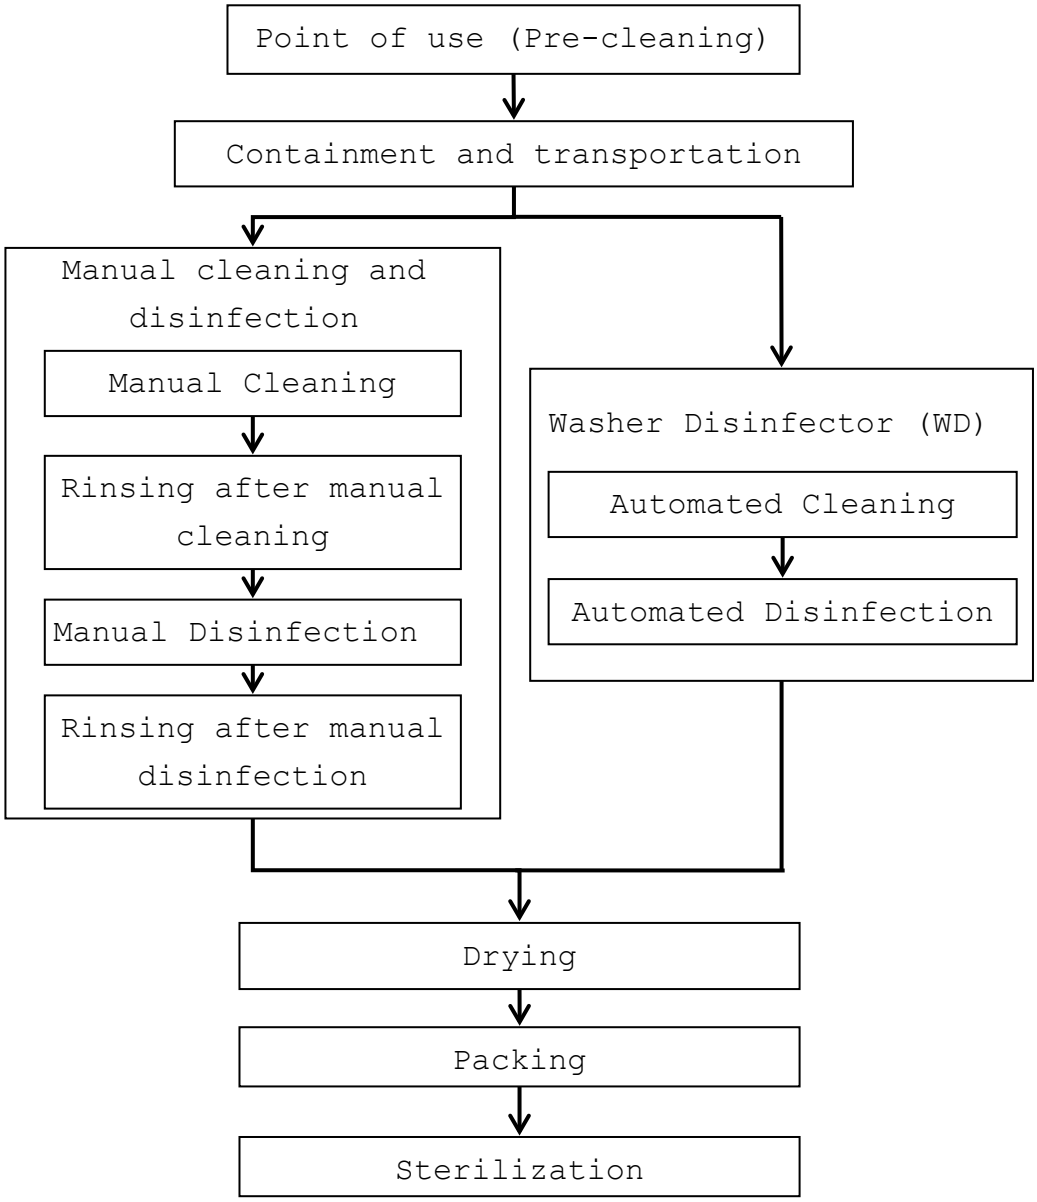

6.1 Point of use (Pre-cleaning)

Point of use (Pre-cleaning)

Pre-cleaning should be done immediately after each use. The procedure is as follows:

1) Remove the EZU-PA3U from the probe.

2) Disassemble the EZU-PA3U (Fig.17) and immerse all parts in sufficient amount of high quality tap water. Scrub them using soft cloth to remove all visible soil and dried protein from their surface.

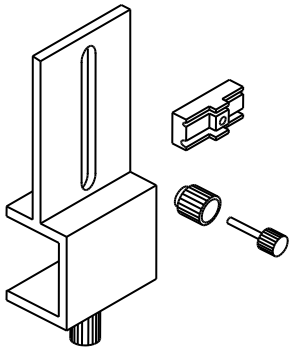


Fig.17 Disassembly of EZU-PA3U

6.2 Containment and transportation

Refer to 5.2.

6.3 Manual Cleaning and disinfection

Manual cleaning and disinfection

Manual Cleaning

↓

Rinsing after manual cleaning

↓

Manual Disinfection

↓

Rinsing after manual disinfection

Prepare following items before manual cleaning and disinfection:

a) Detergent: Cidezyme (Johnson & Johnson, #2258) or another cleaning agent with approved material compatibility for this medical device

b) Disinfectant: Cidex OPA (Johnson & Johnson, # 20391) or another disinfectant with approved material compatibility for this medical device

c) Applicable brush, i.e. REF 09098, REF 09326 (Interlock)

d) Two tanks, one for cleaning and one for disinfection - optional: 1 additional tank for rinsing with deionized/tap water

e) 50 ml syringe

f) Soft, fluff free cloth or single use towel

g) Personal protective equipment (gloves, water repellent protective skirt, face protection mask or protective glasses, see also instructions of the manufacturer for the detergent and the disinfectant)

Manual Cleaning:

Prepare the detergent solution in a tank with cold water (please follow the instructions of the detergent manufacturer regarding application, dilution and contact time).

1) The temperature of the detergent solution should be between 15-30°C (59-86°F), concentration is 1.6%. Please note the minimum contact time of the detergent in the manufacturer's instruction. If a differing detergent is used, please also note the approved material compatibility for the medical device.

2) Immerse the parts of the EZU-PA3U into the diluted detergent solution. Using a syringe flush the cavity of EZU-PA3U 5 times under the surface of the detergent solution. Brush the whole length of EZU-PA3U at least 5 times by using an applicable brush. Brush all parts of EZU-PA3U until they are visually clean.

3) Wipe the parts of the EZU-PA3U under the surface of the detergent solution with a single-use fluff free soft cloth to remove all visible soil. Be sure that all grooves of the EZU-PA3U are implemented during the cleaning process. If necessary use an appropriate brush for this purpose.

4) The parts of the EZU-PA3U should be left in the detergent solution according to the specified contact time of the detergent manufacturer.

5) Rinse the parts of the EZU-PA3U with running tap water for 1 minute. (alternatively: immerse them in a tray filled with deionized water/tap water (see Fig.17) for 5 min. and rinse the cavity of EZU-PA3U with 50 ml tap water. Repeat this 5 times.)

6) Visually check the outer surface of the parts of the EZU-PA3U for cleanness. If necessary, use magnifying glass for visually check. If there is still soil visible, repeat all above steps.

Manual disinfection:


1) Prepare the disinfectant solution as stated in the procedure for the probe.

2) Immerse the parts of the EZU-PA3U into the disinfectant. Rinse the cavity of EZU-PA3U with 50 ml disinfectant solution. Repeat this 4 times. Set a clock to insure the recommended contact time which is 5 minutes.

3) Rinse the parts of the EZU-PA3U with deionized water for 1 minute. (alternatively: immerse them in a tray filled with deionized water for 5 min. and rinse the cavity of EZU-PA3U with 50 ml deionized water. Repeat this 5 times.)

4) Visually check the outer surface of the parts of the EZU-PA3U for leavings of the disinfectant. If necessary, repeat the rinsing.

6.4 Automated cleaning and disinfection

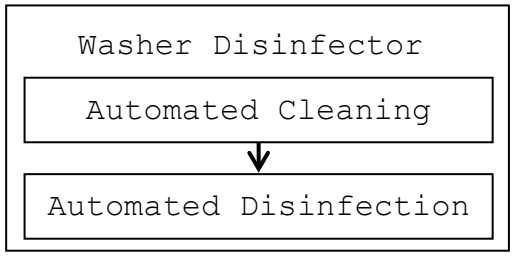

The following items must be provided prior to automated cleaning and disinfection:

a) Washer disinfector: according to DIN EN ISO 15883 with chemo-thermal program

b) Detergent: Korsolex Endo-Cleaner (Bode Chemie; # 972 020) or another cleaning agent with approved material compatibility for this medical device.

c) Disinfectant: Korsolex Endo Disinfectant (Bode Chemie; # 972 030) or another disinfectant with approved material compatibility for this medical device.

d) Washer disinfector accessories:

basket for holding the puncture adapter

basket with lid for holding the dismantled small parts of EZU-PA3U

1) The parameters of the cleaning and disinfection of the device are as follows:

Program step	Water (40 l)	Dosage (ml/l)	Temp. (°C)/(°F)	Time (min)
Pre-Rinse	Cold water	-	-	5
Cleaning	Deionized water	5 (0.5%)	50/122	5
Rinse	Deionized water	-	-	1
Disinfection	Deionized water	10 (1%)	55/131	5
Rinse	Deionized water	-	-	1
Rinse	Deionized water	-	55/131	1
Drying	-	-	55/131	15

2) Place the disassembled parts of EZU-PA3U in the baskets of the washer disinfector. Smaller parts like the screws must be placed in a strainer basket with lid.

3) Close the door of the washer disinfector and start the chemo-thermal program.

4) Open the door after the process is done.

5) Take the parts of EZU-PA3U out of the washer disinfector and check that they are dry. If not, dry them as described in the chapter drying.

6.5 Drying

Drying

Refer to 5.4.

6.6 Inspection

Refer to 5.5.

6.7 Packaging

Packaging

Refer to 5.6.

6.8 Sterilization

Sterilization

EZU-PA3U can be sterilized using ethylen oxide gas (EtO) sterilization plasma sterilization, or Steam sterilization.

Follow the manufacturer's instructions of the sterilizer regarding usage, temperature and sterilization-time.

The sterilization method and operating conditions are as follows.

Sterilization Method	Condition
Plasma Sterilization: STERRAD® 50, 100S or 200 (*)	Short Cycle
Plasma Sterilization: Sterrad® NX or 100NX (*)	Standard cycle
ETO Sterilization	➢ Gas Type: 10% EO/ 90% HCFC ➢ Temperature: 50-55°C 122-131°F ➢ Exposure Time: More than 120 minutes ➢ Pressurization: 162-200kPa Depressurization: 13-8kPa ➢ Relative humidity: 40-90% ➢ Aeration temperature: 53°C 127.4°F ➢ Aeration is minimum 12 hours
Steam Autoclaving (that is applicable to only EZU-PA3U)	➢ Temperature: min. 132°C 269.6°F ➢ Chamber Pressure: 41.7-44.7psia (27-30psig or 3bar) ➢ Exposure time: Minimum 10 minutes.

* STERRAD® systems are manufactured by "Johnson & Johnson"

⚠ WARNING

Before performing sterilization, check that the operation data of sterilizer are in conjunction with min. and max. data applicable for EZU-PA3U.

6.9 Storage

Refer to 5.8.

7 Maintenance and Safety Inspection


7.1 Daily Inspection

7.1.1 Visually inspect the surface of the probe head, housing, cable and connector for any crack, scratch or denaturalization. If you find any damage, do not use the probe and contact one of our company and/or distributor's offices immediately.

7.1.2 Visually inspect the Puncture Guide Fixture for deformation or denaturalization. If you find any damage, do not use the Puncture Guide Fixture and contact one of our company and/or distributor's offices immediately.

7.1.3 Visually inspect the surface of the Magnetic sensor attachment and the Spacer for EZU-RV2S for any crack, deformation or denaturalization. If you find any damage, do not use them and contact one of our company and/or distributor's offices immediately.

7.2 Storage



After using the probe and accessory, they should be cleaned and disinfected/sterilized according to "5. Cleaning, Disinfection and Sterilization" and "6.Cleaning, Disinfection and Sterilization of EZU-PA3U" immediately. Then store them in a cool and dark place avoid high temperature and humidity direct sunlight.

8 Safety Precautions

⚠ WARNING

1) Never use the probe if the probe head, shaft or cable are cracked or damaged.
2) Never use the Puncture Guide Fixture if it is deformed and denaturalized.
3) When use the EUP-U533 for biopsy purpose, use the Puncture Guide Fixture (EZU-PA3U) certainly.
4) Never use the Magnetic sensor attachment and spacer if they are cracked or deformed or denaturalized.
5) The ultrasound gel attached to the ultrasound scanner as one of accessories is not sterile so never use it with EUP-U533.
6) Warning is case of using probe covers which latex is contained to. The latex may cause such allergic reactions as itching, lubor, urticaria, swelling, fever, anhelation, wheezing, depression of blood pressure, shock and so on. For the patients suspected of latex allergy, do not use the latex-containing medical devices. If you observe any of above-mentioned symptoms in your patient during the operation, stop the use of the latex-containing medical devices immediately and take an appropriate treatment to the patient.

⚠ CAUTION

1) Keep the acoustic power low and minimize the ultrasound exposure time for the examination of an early pregnancy.
2) Do not expose the connector to water or other liquids. The connector is not waterproof.
3) Do not hit or drop the probe. The probe is easily damaged by mechanical shock.
4) Do not use detergents and disinfectants other than listed in "9.3 Suppliers list".
5) Use a sterile probe cover to avoid staining or damaging the acoustic lens.
6) Clean, disinfect and sterilize the probe, the Puncture Guide Fixture, the Magnetic sensor attachment and the Spacer for EZU-RV2S before the first use as it is not sterilize in the factory.
7) Use only the soft cloth or tissue to clean the acoustic lens.
8) Only a well-trained physician should perform a biopsy.
9) Do not attach unapproved devices to the probe.
10) The probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S are delivered without being disinfected or sterilized.

9 Specifications

9.1 Probe

Type	: EUP-U533 Transrectal probe
Center frequency	
Convex scanning	: 6.5MHz
Linear scanning	: 7.5MHz
Technology	: High density Convex Array and Linear Array Probe
Dimensions	: See Fig.18
Weight	: Approx. 2kg (incl. cable and connector)
Scanning angle (Convex)	: 200 deg
Field of view (Linear)	: 64mm
Probe materials	: Bio-compatible allergy free components
Acoustic output	: According to IEC 60601-2-37 (See Main Unit manual.)
Applicable system	: Depending on production and upgrade status For detailed information contact one of our company and/or distributor's offices.
Classification	: MDD classification IIa.
Cleaning	: Applicable detergents are listed in the suppliers list
Disinfection	: Applicable disinfectants are listed in the suppliers list
Sterilization	: ETO gas sterilization

Operating conditions:

Ambient temperature	: +25 – +35°C +77 - +95°F
Relative humidity	: 30 – 85%

Storage conditions:

Temperature	: –10 – +55°C +14 - +131°F
Relative humidity	: 10 – 95% (Subject to no condensation)

9.2 Puncture Guide Fixture

Type	: EZU-PA3U
Dimension	: See Fig.19
Materials	: Bio-compatible allergy free components
Classification	: MDD classification IIa
Cleaning	: Applicable detergents are listed in the suppliers list
Sterilization	: Steam Sterilization

Operating conditions:

Temperature	: +5 – +42°C +41 - +107.6°F

Storage conditions:

Temperature	: -10 – +55°C +14 - +131°F
Relative humidity	: 10 – 95%

9.3 Suppliers List

The products listed below are seriously tested and approved for use with the transrectal probe EUP-U533.

Product name	Manufacturer	Purpose
Enzol	Johnson & Johnson	Enzymatic detergent
Meliseptol HBV-Tücher	B Braun	Disinfectant
CIDEX plus	Johnson & Johnson	Disinfectant
Gigasept FF	Schülke & Mayr	Disinfectant
ALKACIDE	ALKAPHARM	Disinfectant
ALKAZYME	ALKAPHARM	Cleaner
Balloon kit, part number: 1450303A	FUJIFILM Healthcare Corporation	Probe cover

Please contact your local distributor for a current version of the "Disinfectant/Sterilization Method Compatibility for Ultrasound Probe and Accessory List

10 Disposal of the probe

Recycle or dispose of equipment properly in compliance with your organizational rules and your local Law.


⚠ CAUTION

Before disposing of equipment, disinfect or take other infection-prevention measures.
Disposal of the equipment without taking the proper preventative measures can lead to infection.

Waste Electrical and Electronic Equipment (WEEE) Directive


The illustration on the right is required by the EU WEEE Directive to appear on all electrical and electronic equipment.
For proper disposal of this product in an EU nation, contact an EU office or agency and observe appropriate local and national regulations and laws.



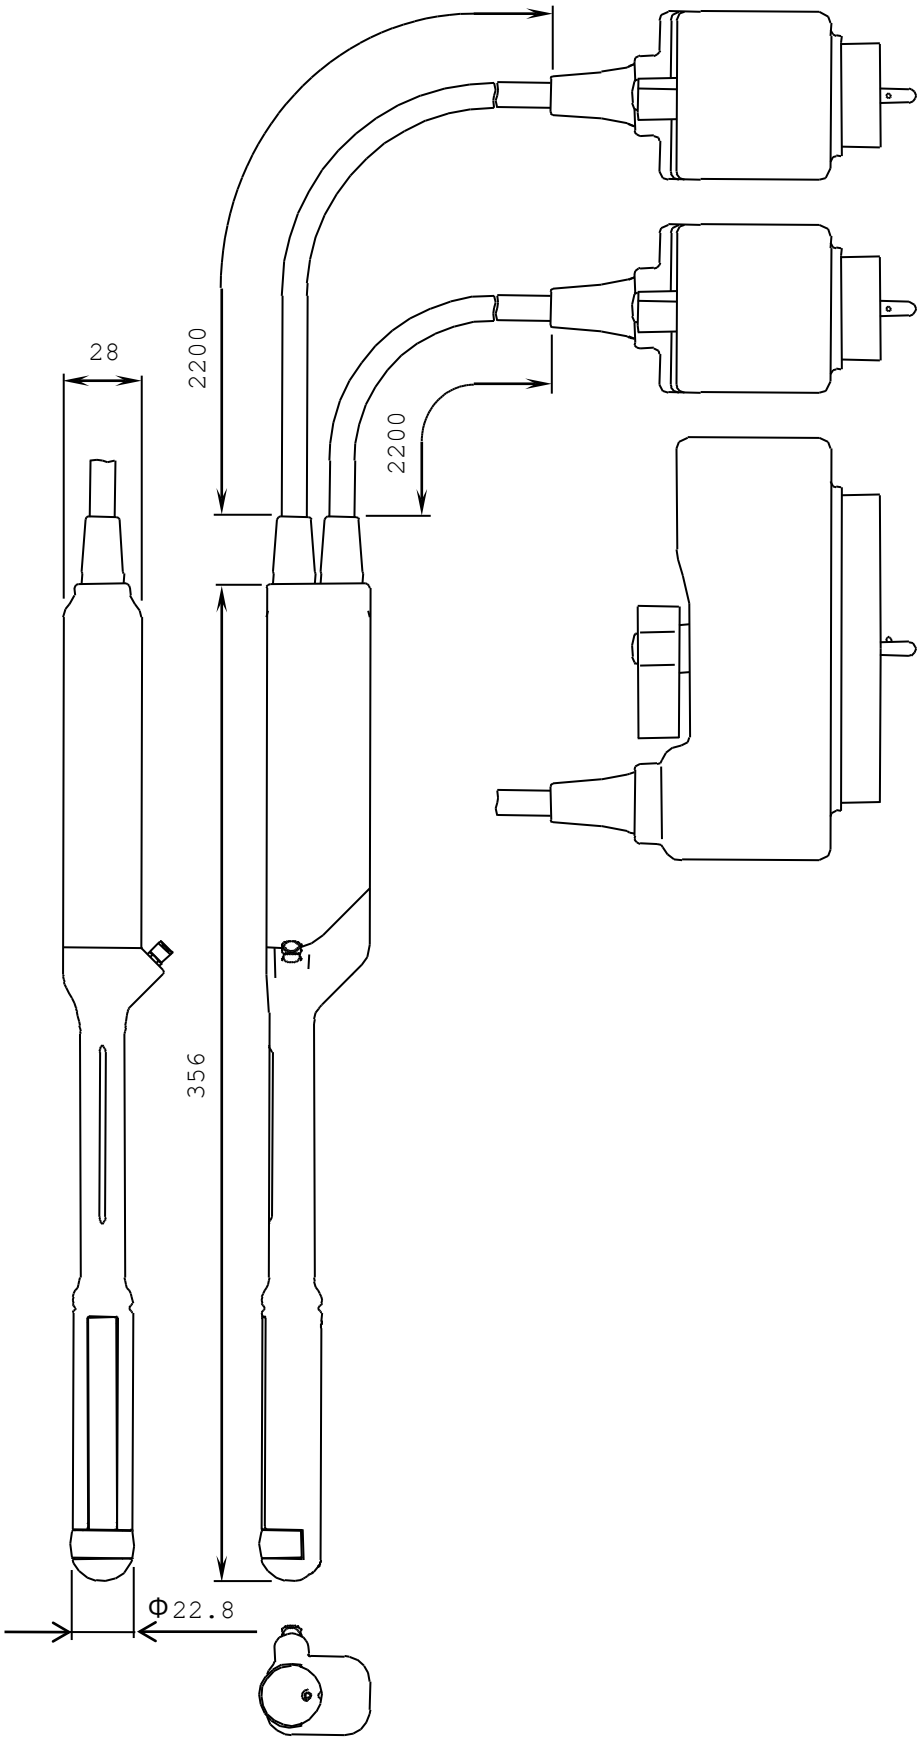

Unit: mm

Fig.18 Dimension Diagram of EUP-U533

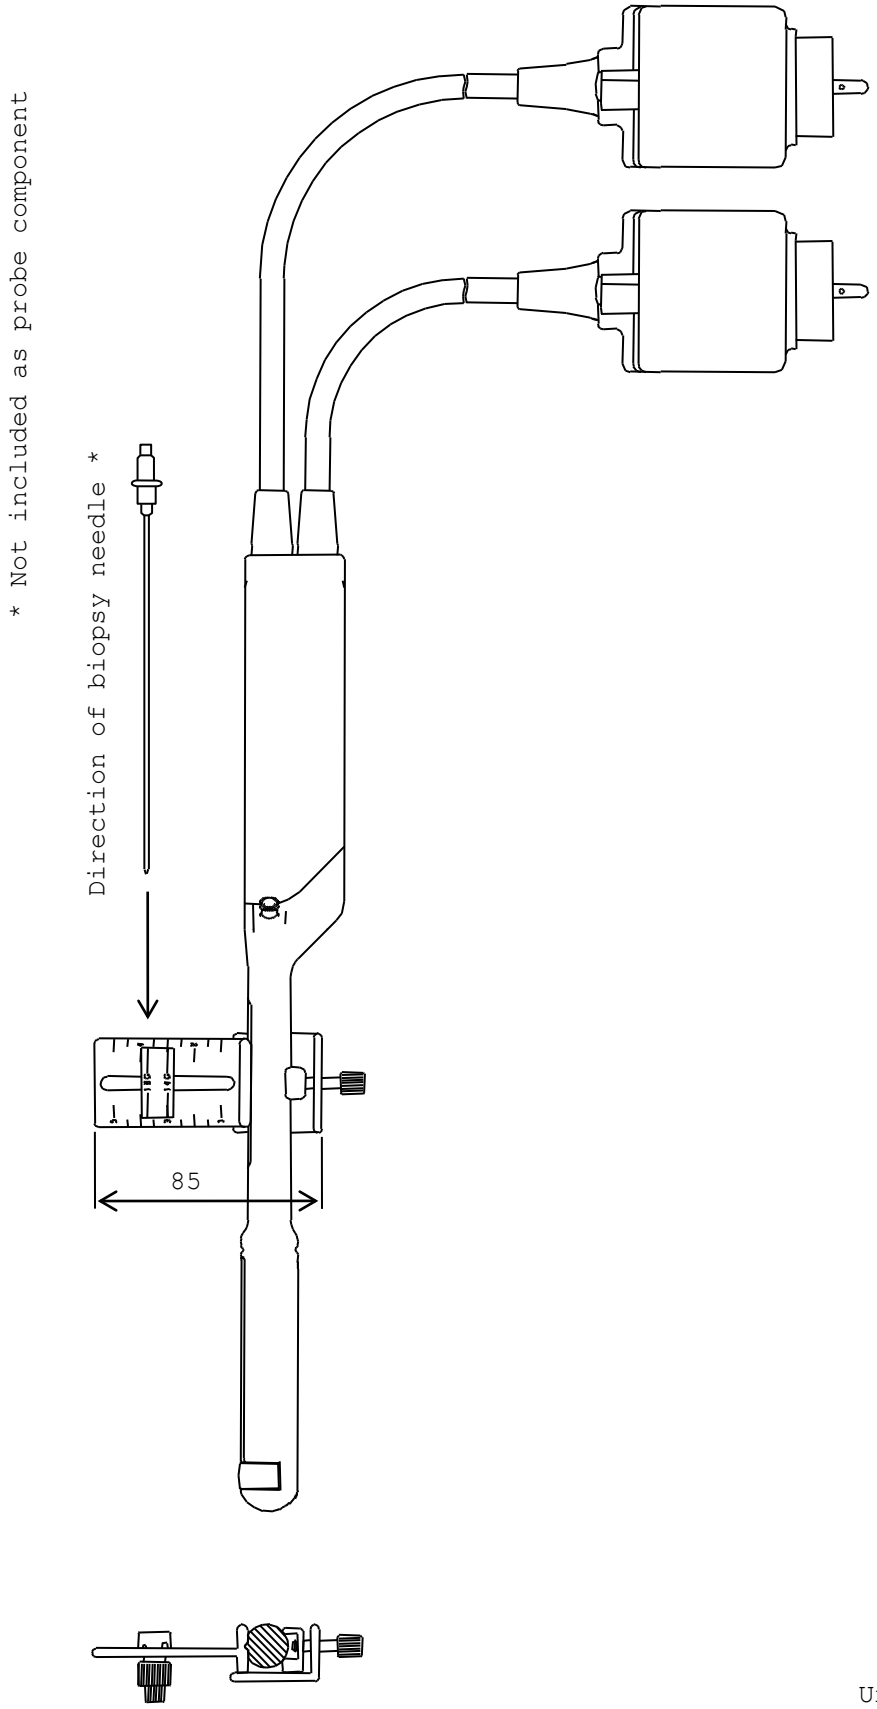

Unit: mm

Fig.19 Dimension Diagram with biopsy adapter (EZU-PA3U)

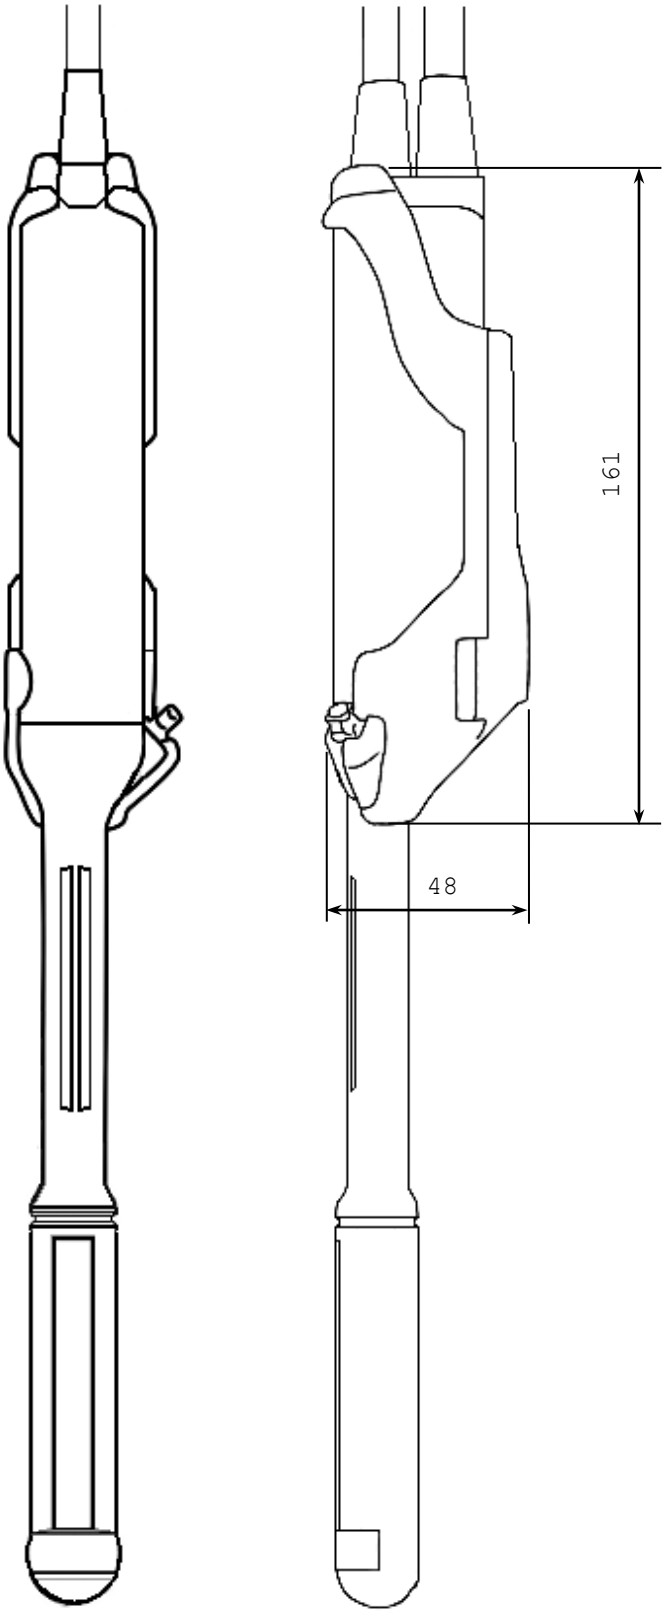


Fig.20 Dimension Diagram with the Magnetic sensor attachment

E